

 **Labor Diagnostika Nord GmbH & Co. KG**

Am Eichenhain 1, 48531 Nordhorn

Telefon: +49-5921-8197 0

Telefax: +49-5921-8197 222

e-mail: manz@ldn.de


Internet: <http://www.ldn.de>



Instructions for use
Progesterone Saliva ELISA **Free**

REF

SA E-6300



IVD



Progesterone Saliva ELISA ^{Free}

Introduction

Intended Use

Enzyme immunoassay for the *in vitro diagnostic* quantitative measurement of active free progesterone (a female hormone) in saliva.

Measurements obtained by this device may be used in the diagnosis and treatment of disorders of the ovaries or placenta and can be used as an aid for prediction of ovulation.

Summary and Explanation

Progesterone (4-pregnene-3, 20-dione) is a C21 steroid hormone containing a keto-group (at C-3) and a double bond between C-4 and C-5. Like other steroids, it is synthesized from cholesterol via a series of enzyme-mediated steps (1)

The steroid hormone Progesterone is a female sex hormone which, in conjunction with estrogens, regulates the accessory organs during the menstrual cycle and it is particularly important in preparing the endometrium for the implantation of the blastocyte and in maintaining pregnancy (2)

In non-pregnant women progesterone is mainly secreted by the corpus luteum whereas in pregnancy the placenta becomes the major source (3,4). Minor sources for progesterone are the adrenal cortex for both sexes and the testes for males.

The Progesterone level in saliva represents the concentration of the active free Progesterone.

PRINCIPLE

The Salivary Progesterone ELISA kit is based on the competition principle and the microplate separation.

An unknown amount of Progesterone present in the sample and a fixed amount of Progesterone conjugated with horseradish peroxidase compete for the binding sites of a rabbit polyclonal Progesterone -antiserum coated onto the wells. After one hour incubation the microplate is washed to stop the competition reaction.

After adding the substrate solution, the concentration of Progesterone is inversely proportional to the optical density measured.

WARNINGS AND PRECAUTIONS

1. For in-vitro diagnostic use only. For professional use only.
2. Before starting the assay, read the instructions completely and carefully. Use the valid version of the package insert provided with the kit. Be sure that everything is understood.
3. Do not mix reagents of different lots. Do not use expired reagents.
4. The microplate contains snap-off strips. Unused wells must be stored at 2 – 8°C in the sealed foil pouch and used in the frame provided.
5. Avoid contact with Stop Solution, 0.5M H₂SO₄. It may cause skin irritation and burns.
6. Pipetting of samples and reagents must be done as quickly as possible and in the same sequence for each step.
7. Use separate pipette tips for each sample, control and reagent to avoid cross contamination.
8. Use reservoirs only for single reagents. This especially applies to the substrate reservoirs. Using a reservoir for dispensing a substrate solution that had previously been used for the conjugate solution may turn solution colored. Do not pour reagents back into vials as reagent contamination may occur.
9. Mix the contents of the microplate wells thoroughly to ensure good test results. Do not reuse microwells.
10. Do not let wells dry during assay; add reagents immediately after completing the rinsing steps.
11. Kit calibrators have been checked for HIV-1/2 and HCV antibodies and HBsAg and found to be negative, but the calibrators and patient samples should be handled as potentially infectious.
12. Some reagents contain Proclin, BND and MIT as preservatives. In case of contact with eyes or skin, flush immediately with water.
13. Allow the reagents to reach room temperature (21-26°C) before starting the test. Temperature will affect the absorbance readings of the assay. However, Values for the patient samples will not be affected.
14. TMB substrate has an irritant effect on skin and mucosa. In case of possible contact, wash eyes with an abundant volume of water and skin with soap and abundant water. Wash contaminated objects before reusing them. If inhaled, take the person to open air.

REAGENTS

Reagents provided

96

SA E-6331 Microtiterwells

12x8 (break apart) strips, 96 wells; Wells coated with a anti-Progesterone antibody (polyclonal).

Standards

	Cat. no.	Standard	Concentration	Volume/Vial
STANDARD A	SA E-6301	Standard 0	0 pg/mL	1 ml
STANDARD B	SA E-6302	Standard 1	10 pg/mL	1 ml
STANDARD C	SA E-6303	Standard 2	50 pg/mL	1 ml
STANDARD D	SA E-6304	Standard 3	100 pg/mL	1 ml
STANDARD E	SA E-6305	Standard 4	500 pg/mL	1 ml
STANDARD F	SA E-6306	Standard 5	1000 pg/mL	1 ml
STANDARD G	SA E-6307	Standard 6	5000 pg/mL	1 mL

Conversion: 1000 pg/mL x 3.18 = nmol/L.

* contain 0.03% Proclin 300, 0.015% BND and 0.010% MIT as preservatives.

CONTROL 1

+ CONTROL 2

SA E-6351 + SA E-6352 Control

2 vials, 1.0 mL each, ready to use; Control values and ranges please refer to vial label or QC-Datasheet.

* contain 0.03% Proclin 300, 0.015% BND and 0.010% MIT as preservatives.

CONJUGATE

SA E-6340 Enzyme Conjugate

1 vial, 26 mL, ready to use; Progesterone conjugated to horseradish peroxidase;

* contain 0.03% Proclin 300, 0.015% BND and 0.010% MIT as preservatives.

SUBSTRATE

SA E-0055 Substrate Solution

1 vial, 25 mL, ready to use; Tetramethylbenzidine (TMB).

STOP-SOLN

FR E-0080 Stop Solution

1 vial, 14 mL, ready to use; contains 0.5M H₂SO₄.

Avoid contact with the stop solution. It may cause skin irritations and burns.

WASH-CONC 40x

FR E-0030 Wash Solution

1 vial, 30 mL (40X concentrated); see „Preparation of Reagents“.

* BND = 5-bromo-5-nitro-1,3-dioxane

MIT = 2-methyl-2H-isothiazol-3-one

Note: Additional *Standard 0* for sample dilution is available upon request.

Materials required but not provided

1. Calibrated EIA reader adjusted to read at 450 nm
2. Precision pipettes (100 and 200 µl)
3. Distilled or Deionized water
4. Timer (60 min. range)
5. Reservoirs (disposable)
6. Test tube or microtube rack in a microplate configuration
7. semi logarithmic graph paper or software for data reduction

Storage Conditions

When stored at 2 °C to 8 °C unopened reagents will retain reactivity until expiration date. Do not use reagents beyond this date.

Opened reagents must be stored at 2 °C to 8 °C. Microtiter wells must be stored at 2 °C to 8 °C. Once the foil bag has been opened, care should be taken to close it tightly again.

Opened kits retain activity for two months if stored as described above.

Reagent Preparation

Bring all reagents to room temperature before use.

Wash Solution

Add deionized water to the 40X concentrated *Wash Solution*.

Dilute 30 mL of concentrated *Wash Solution* with 1170 mL deionized water to a final volume of 1200 mL.

The diluted Wash Solution is stable for 2 weeks at room temperature.

SPECIMEN Collection and Preparation

Eating, drinking, chewing gums or brushing teeth should be avoided for 30 minutes before sampling. Otherwise, it is recommended to rinse mouth thoroughly with cold water 5 minutes prior to sampling.

Do not collect samples when oral diseases, inflammation or lesions exist (blood contamination).

If there is visible blood contamination the patient specimen, it should be discarded, rinse the sampling device with water, wait for 10 minutes and take a new sample.

Note: Samples containing sodium azide should not be used in the assay.

Specimen Collection

It is recommended to collect saliva samples with commercially available equipment (e.g. SALI SET 100 REF SA D-6100 available from LDN).

Do not use any PE devices or Salivettes for sampling; this in most cases will result in significant interferences. Glas tubes can be used as well, but in this case special attention is necessary for excluding any interference caused by the stopper.

As the Progesterone secretion in saliva as well in serum shows an obvious episodic secretion pattern it is important to care for a proper timing of the sampling.

In order to avoid arbitrary results we are recommending to always take 5 samples within a period of 2 – 3 hours (multiple sampling) preferably before a meal.

As food might contain significant amounts of steroid hormones samples preferably should be taken while fasting. If fasting should be a problem the collection period should be timed just before lunch or before dinner.

Specimen Storage and Preparation

Saliva samples in general are stable at ambient temperature for several days.

Therefore mailing of such samples by ordinary mail without cooling will not create a problem.

Storage at 4°C can be done for a period of up to one week.

Whenever possible samples preferable should be kept at a temperature of -20°C.

Even repeated thawing and freezing is no problem.

Each sample has to be frozen, thawed, and centrifuged at least once anyhow in order to separate the mucins by centrifugation.

Upon arrival of the samples in the lab the samples have to stay in the deep freeze at least overnight. Next morning the frozen samples are warmed up to room temperature and mixed carefully.

Then the samples have to be centrifuged for 5 to 10 minutes.

Now the clear colorless supernatant is easy to pipette.

If the sample should show even a slighty reddish color it should be discarded. Otherwise the value most probably will be falsely elevated.

At least during the luteal phase of females there is a significant episodic excretion pattern of Progesterone. Due to this episodic variation of the steroid secretion we highly recommend the strategy of multiple sampling.

If such a set of multiple samples have to be tested the lab (after at least one freezing, thawing, and centrifugation cycle) has to mix the aliquots of the 5 single samples in a separate sampling device and perform the testing from this mixture.

Specimen Dilution

If in an initial assay, a specimen is found to contain more than the highest standard, the specimens can be diluted with *Standard 0* solution and re-assayed as described in Assay Procedure.

For the calculation of the concentrations this dilution factor has to be taken into account.

Example:

a) Dilution 1:10: 10 µl saliva + 90 µl *Standard 0* (mix thoroughly)

b) Dilution 1:100: 10 µl of dilution a) + 90 µl *Standard 0* (mix thoroughly).

ASSAY PROCEDURE

General Remarks

- All reagents and specimens must be allowed to come to room temperature before use. All reagents must be mixed without foaming.
- Once the test has been started, all steps should be completed without interruption.
- Use new disposal plastic pipette tips for each standard, control or sample in order to avoid cross contamination.
- Absorbance is a function of the incubation time and temperature. Before starting the assay, it is recommended that all reagents are ready, caps removed, all needed wells secured in holder, etc. This will ensure equal elapsed time for each pipetting step without interruption.
- As a general rule the enzymatic reaction is linearly proportional to time and temperature.

Assay Procedure

Each run must include a standard curve.

1.	Secure the desired number of coated strips in the frame holder.
2.	Dispense 100 µl of each Progesterone Standards and Controls into appropriate wells.
3.	Dispense 100 µl of each sample into selected wells.
4.	Dispense 200 µl of Enzyme Conjugate into each sample and standard well and mix the plate for thoroughly for 10 seconds.
5.	Incubate for 60 minutes at room temperature.
6.	Briskly shake out the contents of the wells and rinse the wells 3 times with diluted Wash Solution (400 µl per well). Strike the inverted wells sharply on absorbent paper towel to remove residual droplets. Important note: The sensitivity and precision of this assay is markedly influenced by the correct performance of the washing procedure!
7.	Add 200 µl of Substrate Solution to each well.
8.	Incubate for 15 minutes at room temperature.
9.	Stop the reaction by adding 100 µl of Stop Solution to each well.
10.	Determine the absorbance of each well at $450 \pm \square 10$ nm. It is recommended to read the wells within 10 minutes.

Calculation of Results

1. Calculate the average absorbance values for each set of standards, controls and patient samples.
2. Construct a standard curve by plotting the mean absorbance obtained from each standard against its concentration with absorbance value on the vertical(Y) axis and concentration on the horizontal (X) axis.
3. Using the mean absorbance value for each sample determine the corresponding concentration from the standard curve.
4. Automated method: The results in the IFU have been calculated automatically using a 4 PL (4 Parameter Logistics) curve fit. 4 Parameter Logistics is the preferred calculation method. Other data reduction functions may give slightly different results.
5. The concentration of the samples can be read directly from this standard curve. Samples with concentrations higher than that of the highest standard have to be further diluted. For the calculation of the concentrations this dilution factor has to be taken into account.

Conversion:

Progesterone Conversion: $1000 \text{ pg/mL} \times 3.18 = \text{nmol/L}$.

Example of Typical Standard Curve

The following data is for demonstration only and cannot be used in place of data generation at the time of assay.

Standard	Absorbance Units (450 nm)
Standard 0 (0 pg/mL)	1.89
Standard 1 (10 pg/mL)	1.71
Standard 2 (50 pg/mL)	1.54
Standard 3 (100 pg/mL)	1.39
Standard 4 (500 pg/mL)	0.95
Standard 5 (1000 pg/mL)	0.71
Standard 6 (5000 pg/mL)	0.44

EXPECTED NORMAL VALUES

In order to determine the normal range of SLV Progesterone, saliva samples from 80 adult male and 120 female apparently healthy subjects, ages 21 to 75 years, were collected in the morning and analyzed using the Progesterone ELISA kit.

The following ranges were calculated from this study.

	Age group	n	Salivary progesterone pg/mL
Women	21 - 50 yrs. Follicular phase	40	19.6 – 86.5 pg/mL
	21 - 50 yrs. Luteal phase	40	99.1 – 332.6 pg/mL
	51 - 75 yrs. Postmenopausal	40	6.0 – 56.4 pg/mL
Men	21 - 50 yrs.	40	12.7 – 57.4 pg/mL
	51 - 75 yrs.	40	15.2 – 65.1 pg/mL

Therapy should not be decided based on results alone. The results should be correlated to other clinical observations and diagnostic tests.

Furthermore, we recommend that each laboratory establish its own range for the population tested, because the values differ between age, new born, children, adolescents and adults.

Quality Control

Good laboratory practice requires that controls be run with each calibration curve. A statistically significant number of controls should be assayed to establish mean values and acceptable ranges to assure proper performance.

It is recommended to use control samples according to state and federal regulations. The use of control samples is advised to assure the day to day validity of results. Use controls at both normal and pathological levels. The controls and the corresponding results of the QC-Laboratory are stated in the QC certificate added to the kit. The values and ranges stated on the QC sheet always refer to the current kit lot and should be used for direct comparison of the results.

It is also recommended to make use of national or international Quality Assessment programs in order to ensure the accuracy of the results.

Employ appropriate statistical methods for analysing control values and trends. If the results of the assay do not fit to the established acceptable ranges of control materials patient results should be considered invalid.

In this case, please check the following technical areas: Pipetting and timing devices; photometer, expiration dates of reagents, storage and incubation conditions, aspiration and washing methods.

After checking the above mentioned items without finding any error contact your distributor or the manufacture directly.

PERFORMANCE CHARACTERISTICS

Sensitivity

The lowest detectable level of progesterone that can be distinguished from the Zero Standard is 3.8 pg/mL at the 95 % confidence limit.

Specificity

The following materials have been evaluated for cross reactivity. The percentage indicates cross reactivity at 50% displacement compared to Progesterone.

Steroid	% cross reactivity
Progesterone	100.0
Desoxycorticosterone	1.1
Pregnenolone	0.35
17 α -Hydroxyprogesterone	0.3
Corticosterone	0.2
11-Desoxycortisol	0.1
Estriol	<0.1
Estradiol 17 β	<0.1
Testosterone	<0.1
Cortisone	<0.1
DHEA-S	<0.02
Cortisol	<0.02

Reproducibility

Intra-Assay

The intra-assay variation was determined by 20 replicate measurements of 5 saliva samples within one run. The within-assay variability is shown below:

Mean (pg/mL)	1328.7	650.1	293.8	186.9	23.3
SD (pg/mL)	75.9	30.4	15.8	10.6	1.8
CV (%)	5.7	4.7	5.4	5.7	7.6
n =	20	20	20	20	20

Inter-Assay

The inter-assay (between-day) variation was determined by duplicate measurements of 5 saliva samples over 10 days.

Mean (pg/mL)	55.5	565.4	1338.0	567.9	630.6
SD (pg/mL)	4.3	41.5	70.9	40.5	45.1
CV (%)	7.7	7.3	5.3	7.1	7.2
n =	20	20	20	20	20

Inter-Lot

The Inter-Lot (between-lot) variation was determined by triplicate measurements of five saliva samples in three different kit lots. The between lot variability is shown below:

Mean (pg/mL)	60.4	630.3	1574.8	360.3	635.1
SD (pg/mL)	4.3	37.6	64.1	28.7	33.4
CV%	7.1	6.0	4.1	8.0	5.3
n=	9	9	9	9	9

Recovery

Recovery of the Progesterone ELISA was determined by adding increasing amounts of the analyte to five different saliva samples containing different amounts of endogenous analyte. Each sample (native and spiked) was assayed and analyte concentrations of the samples were calculated from the standard curve. The percentage recoveries were determined by comparing expected and measured values of the samples

	Sample 1	Sample 2	Sample 3	Sample 4	Sample 5
Concentration pg/mL	13.9	87.9	147.8	283.0	386.8
Average % recovery	96.4	103.2	100.3	97.3	102.2
Range of from % recovery to	91.1 101.6	101.1 104.8	94.9 103.8	92.7 106.6	97.8 105.7

Linearity

In total six saliva samples containing different amounts of analyte were serially diluted with Standard 0 and assayed with this ELISA.

Three of these samples were serially diluted directly, and the other 3 samples at first were spiked with progesterone and then serially diluted up to 1:128.


The percentage recovery was calculated by comparing the expected and measured values for progesterone. A linearity of 3.8 – 4600 pg/mL has been identified as the usable range for this assay. Samples above this range must be diluted and re-run.

	Sample 1	Sample 2	Sample 3	Sample 4	Sample 5	Sample 6
Concentration (pg/mL)	58.3	98.7	1073	2802	6000	5000
Average % Recovery	104.1	97.5	95.79	98.96	102.6	103.5
Range of from Recovery % to	99.9 106.7	89.9 100.8	91.2 105.5	93.6 107.3	99.1 106.5	94.4 107.7

Comparison Studies

A study was performed that evaluated 306 saliva samples collected from adult men and women ages 20 – 75. The samples were run on the test and a commercially available LIA method to determine the concentration of free progesterone in the saliva samples. A correlation of 0.9373 and regression formula of $y = 0.912x + 6.066$ was obtained versus this method.

An additional study was performed using 101 saliva samples from adult men and women ages 20 - 75. These samples were compared to the LIA method, and yielded a correlation of $r = 0.9923$ with the following regression formula.

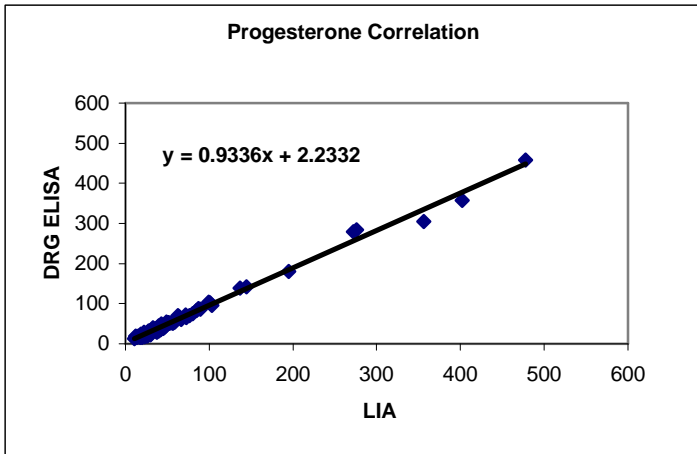

LIMITATIONS OF PROCEDURE

Reliable and reproducible results will be obtained when the assay procedure is performed with a complete understanding of the package insert instruction and with adherence to good laboratory practice. Blood contamination of more than 0.16% in saliva samples will affect results, and usually can be seen by eye. Concentrations of Sodium Azide $\geq 0.02\%$ interferes in this assay and may lead to false results.

REFERENCES

1. Miller W.L. (1988): Molecular biology of steroid hormone synthesis, *Endocrin. Rev.* 9, 295-318
2. Filicori M., Butler J.P., Crowley W.F. Jr. (1984): Neuroendocrine regulation of the corpus luteum in the human, *J. Clin. Invest.* 73, 1638
3. Csapol Al., Pulkkinen M. O., Wiest W.G. (1973): Effects of lutectomy and progesterone replacement therapy in early pregnancy patients. *Am J. Obstet. Gynecol.* 115, 759
4. Henson M.C. (1998): Pregnancy maintenance and the regulation of placental progesterone biosynthesis in the baboon. *Human Reproduction Update*, 4, 389-405

Symbols:

	Storage temperature		Manufacturer		Contains sufficient for <n> tests
	Expiry date	LOT	Batch code	IVD	For in-vitro diagnostic use only!
	Consult instructions for use	CONT	Content	CE	CE labelled
	Caution	REF	Catalogue number	RUO	For research use only!